


## Supplementary Information

### Evaluation of Turbidimetric and Nephelometric Techniques for Analytical Determination of *N*-Acetylcysteine and Thiamine in Pharmaceutical Formulations Employing a Lab-Made Portable Microcontrolled Turbidimeter and Nephelometer


Vagner B. dos Santos,<sup>a</sup> Thiago B. Guerreiro,<sup>a</sup> Willian T. Suarez,<sup>b</sup> Ronaldo C. Faria<sup>a</sup> and Orlando Fatibello-Filho<sup>\*,a</sup>

<sup>a</sup>Departamento de Química, Universidade Federal de São Carlos, Centro de Ciências Exatas e de Tecnologia, CP 676, 13560-970 São Carlos-SP, Brazil

<sup>b</sup>Departamento de Química, Universidade Federal de Viçosa, Centro de Ciências Exatas e Tecnológicas, 36570-000 Viçosa-MG, Brazil

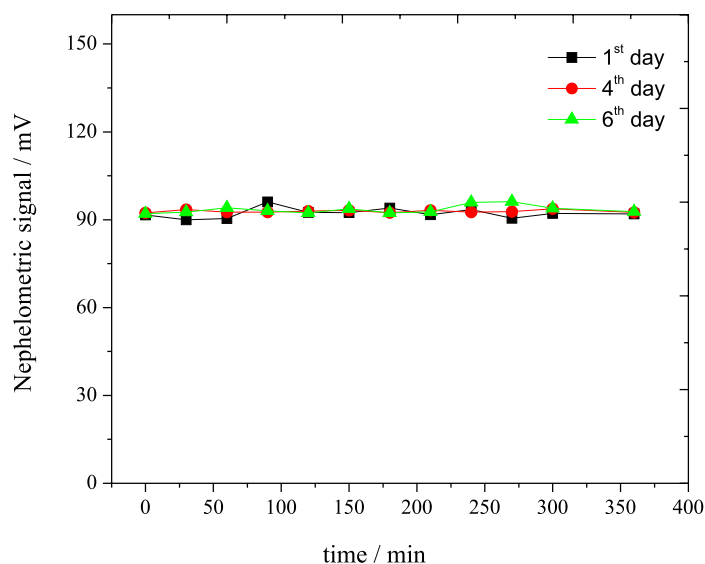

**Figure S1.** Evaluation of the stability of PMTN. Monitoring performed for a period of 6 h on three different days. Only nephelometric data in mV are shown (465 nm).

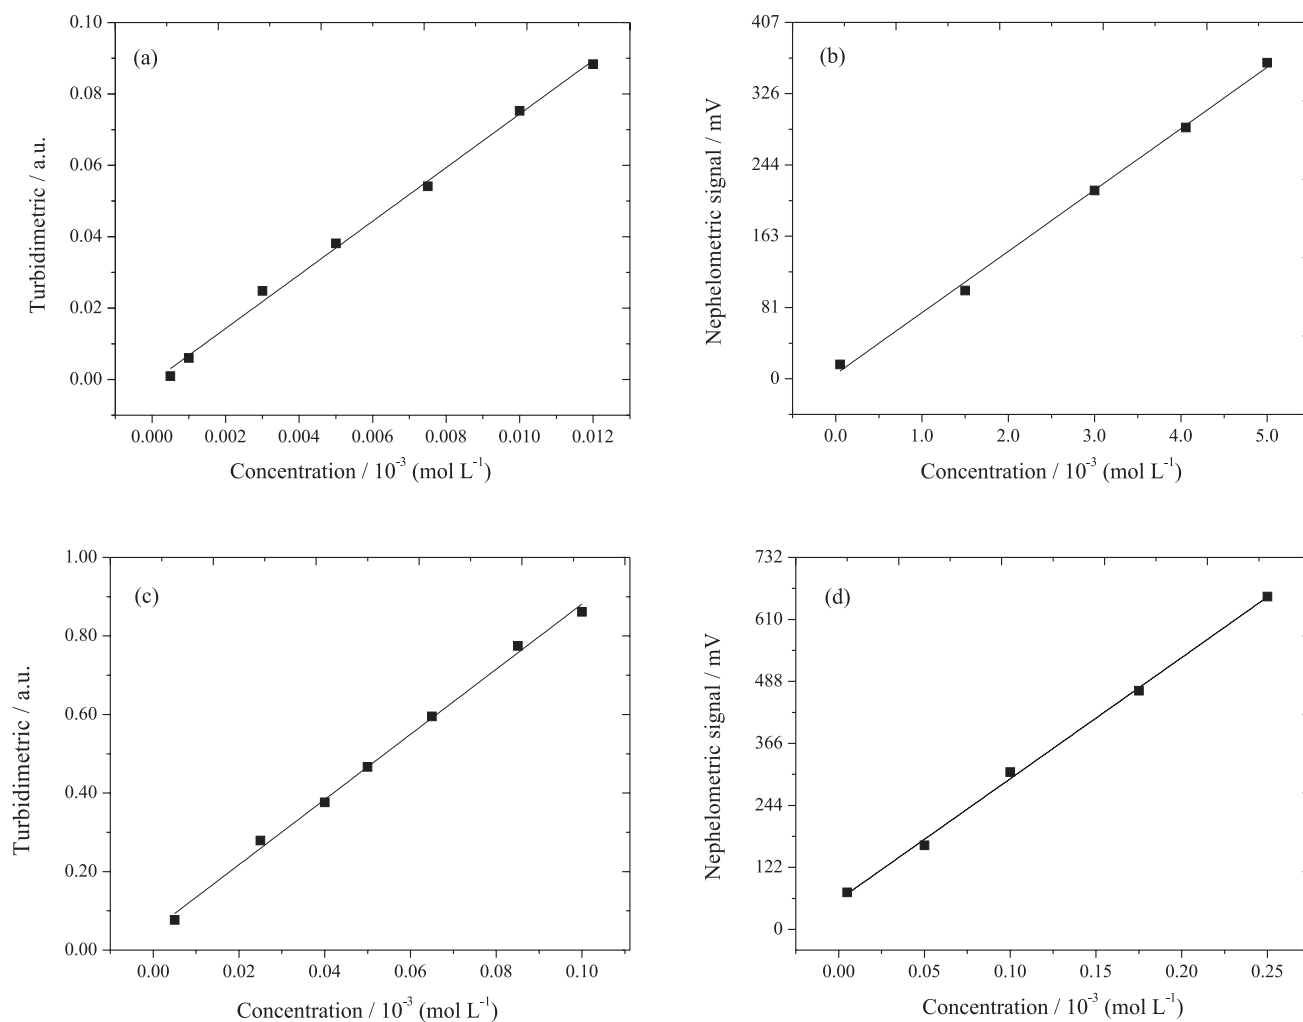

**Figure S2.** Analytical curves for *N*-acetylcysteine in the (a) turbidimetric and (b) nephelometric analyses. Analytical curves for thiamine with (c) turbidimetric and (d) nephelometric detections. All the measurements were performed at 465 nm.